



**CERTIFIED WEIGHT REPORT**

**Part Number:** 79205  
**Lot Number:** 061121  
**Description:** Chrysene

**Solvent:** Acetone  
**Lot#:** 81025

**Expiration Date:** 061126  
**Recommended Storage:** Refrigerate (4 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test ID#:** 6UTB



Weight(s) shown below were combined and diluted to (mL): 25.0 0.005  
Balance Uncertainty  
Flask Uncertainty

**CAUTION: Sonicate Before Use**

		061121
Formulated By:	Prashant Chauhan	DATE
		061121
Reviewed By:	Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Chrysene	91	012015	1000	98	0.2	0.02551	0.02561	1004.1	5.7	218-01-9	0.2mg/m3	N/A

**Method GC8MSD-2.M:** Column:SBB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (14 min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 290°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Nicole Poisson

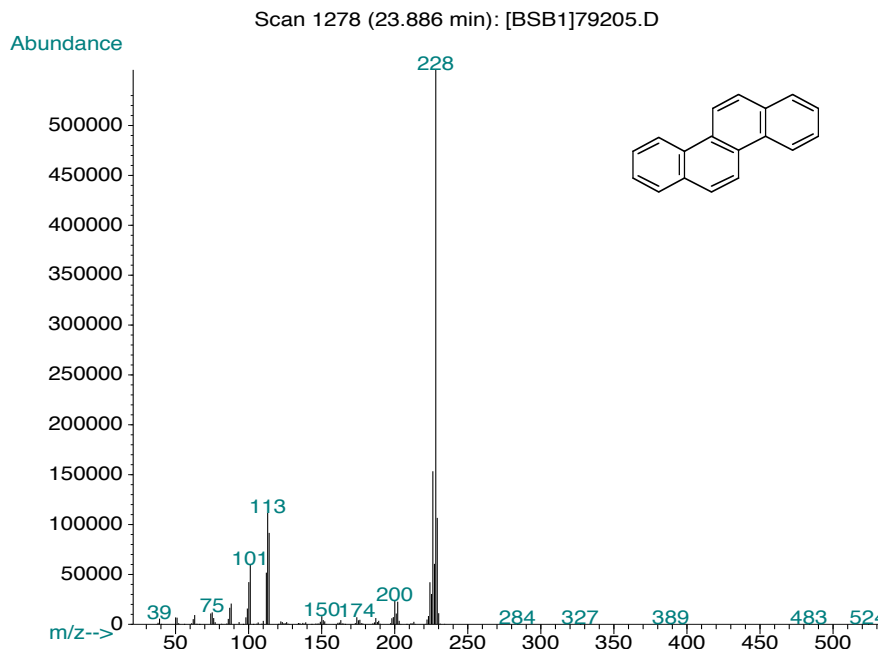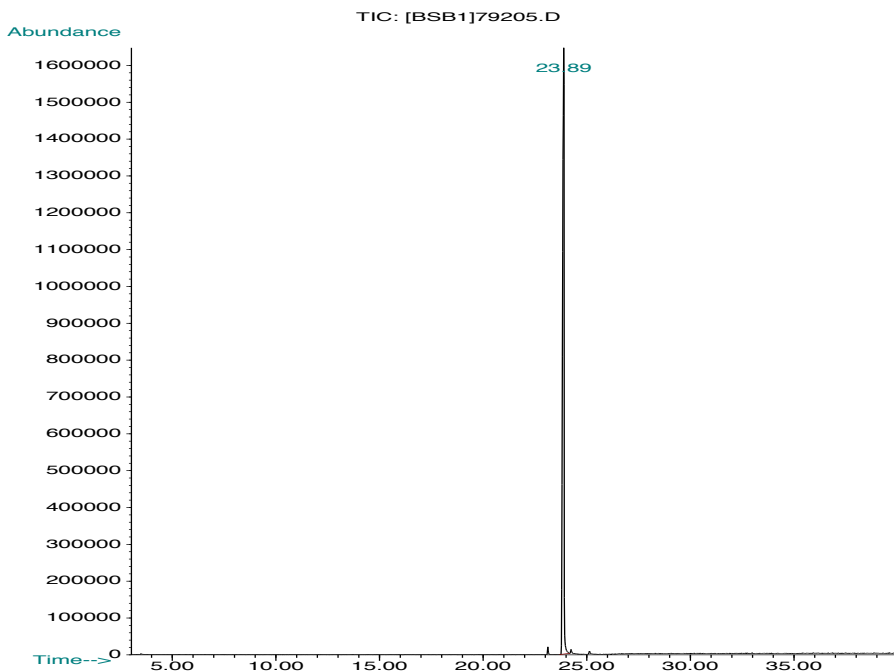

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).